

The following sample(s) was/were submitted and identified on behalf of the client as:

Consignor : ELASTRON PORTUGAL, SA
 Consignor address : RUA DA RECTA DE GOMIL, N°354-ARMAZEM A2 4595-144 F RAZAO PACOS DE FERREIRA-PORTUGAL
 Sample description : White KN95 mask
 Color : (A)white
 No of Sample : (A)50
 Judgement Accordance : GB 2626-2019 Respiratory protective – Non-powered air-purifying particle respirator
 Test Type : Submitted (sample sent by client)

Sample Receiving Date : Oct 15, 2020
 Testing Period : Oct 15, 2020 - Nov 02, 2020
 Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the sample(s) tested, for further details, please refer to the following page(s).

Signed for and on behalf of
 SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center

Ellen Cui (Authorized Signatory)

This test report refer only to the samples tested

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

3rd Building, No.889, Yishan Road, Xuhui District Shanghai, China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgs.com.cn
 中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com



Test Result

Exhalation Resistance

(GB 2626-2019, 6.6;)

	Unit	A	Requirement
As Received			-
Result 1#	Pa	144.4	<=210
Result 2#	Pa	141.1	<=210
After temperature and humidity pretreatment			-
Result 1#	Pa	132.0	<=210
Result 2#	Pa	135.6	<=210
Conclusion		PASS	

Filtration Efficiency

(GB 2626-2019, 6.3; NaCl aerosol)

	Unit	A	Requirement
As Received			-
Result 1#	%	98.009	>=95.0
Result 2#	%	98.847	>=95.0
Result 3#	%	98.670	>=95.0
Result 4#	%	97.860	>=95.0
Result 5#	%	97.841	>=95.0
Result 6#	%	96.567	>=95.0
Result 7#	%	95.395	>=95.0
Result 8#	%	97.298	>=95.0
Result 9#	%	98.756	>=95.0
Result 10#	%	97.245	>=95.0
Result 11#	%	97.586	>=95.0
Result 12#	%	96.735	>=95.0
Result 13#	%	95.687	>=95.0
Result 14#	%	97.535	>=95.0
Result 15#	%	98.166	>=95.0
After temperature and humidity pretreatment			-
Result 1#	%	95.267	>=95.0
Result 2#	%	96.105	>=95.0
Result 3#	%	95.983	>=95.0
Result 4#	%	95.570	>=95.0
Result 5#	%	95.695	>=95.0
Conclusion		PASS	

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com




Inhalation Resistance

(GB 2626-2019, 6.5;)

	Unit	A	Requirement
As Received			-
Result 1#	Pa	150.0	<=210
Result 2#	Pa	148.2	<=210
After temperature and humidity pretreatment			-
Result 1#	Pa	140.1	<=210
Result 2#	Pa	137.7	<=210
Conclusion		PASS	

Sample Photo

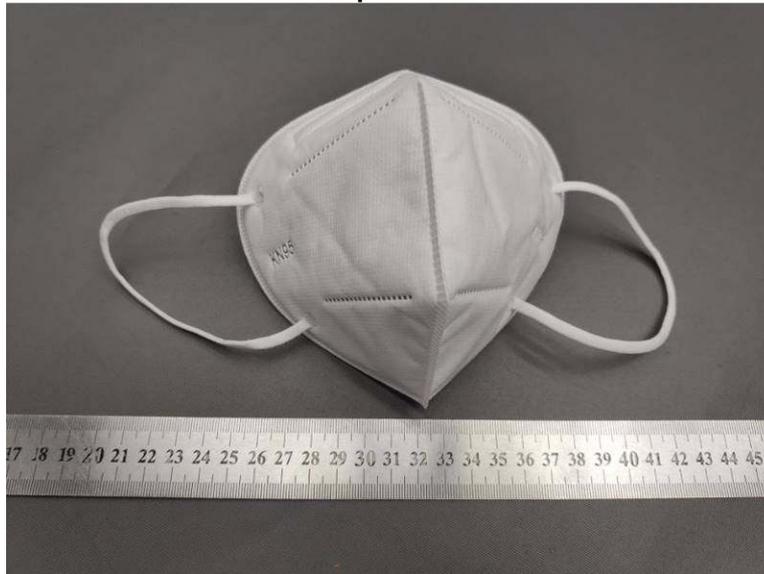

The statement of conformity in this test report is only based on measured values by the laboratory and does not take their uncertainties into consideration.

End of Report



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 3rd Building, No.889, Yishan Road, Xuhui District Shanghai, China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn
 中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com